




## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<b>(51) International Patent Classification 5 :</b>  <b>A61M 5/28</b>	<b>A1</b>	<b>(11) International Publication Number:</b> <b>WO 93/09825</b>  <b>(43) International Publication Date:</b> 27 May 1993 (27.05.93)
<b>(21) International Application Number:</b> PCT/CA92/00495 <b>(22) International Filing Date:</b> 13 November 1992 (13.11.92)  <b>(30) Priority data:</b> 791,399 14 November 1991 (14.11.91) US  <b>(71) Applicant:</b> DUOJECT MEDICAL SYSTEMS INC. [CA/CA]; P.O. Box 600, 305 Knowlton Road, Lac Brome, Quebec J0E 1VO (CA).  <b>(72) Inventor:</b> REYNOLDS, David, L. ; P.O. Box 600, 305 Knowlton Road, Lac Brome, Quebec J0E 1VO (CA).  <b>(74) Agent:</b> PARSONS, Richard, A., R.; Ridout & Maybee, 2300 Richmond-Adelaide Centre, 101 Richmond Street West, Toronto, Ontario M5H 2J7 (CA).		<b>(81) Designated States:</b> AU, BB, BG, BR, CA, CS, DE, FI, GB, HU, JP, KR, NO, RO, RU, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, SE).  <b>Published</b> <i>With international search report.</i> <i>Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i>
<b>(54) Title:</b> SYRINGE  <b>(57) Abstract</b>  <p>A prefilled syringe system is provided for two component pharmaceuticals, which is a combination of a first subassembly consisting of a capped bottomless pharmaceutical vial (2) containing a first component and closed at its bottom end by a piston (32) which can be connected to a plunger (16) and a second subassembly (3) consisting of a shell (4) containing a second component and closed by a further piston (6) and located in telescopic relationship with the plunger, a cap (18) which can be forced onto the cap (36) of the bottomless vial, and a double ended needle (320) or a functionally equivalent cannula assembly which is caused to pierce both pistons as the assemblies are connected by forcing the cap (18) onto the bottomless vial, thus placing the vials in communication. The shell vial (4) is pressed towards the bottomless vial (2) to express its contents into the latter, and the plunger (16) and shell vial (4) are then removed so that the cap (18) and needle (20) are left connected to the bottomless vial (2) and the plunger (16) may be connected to the piston (32) of the bottomless vial to convert it into a syringe. The shell vial may telescope either over or within the plunger. In the first case, the plunger acts to operate the piston of the shell vial during expression of its contents, whereas in the latter case a separate component (8) is required for this purpose.</p>		

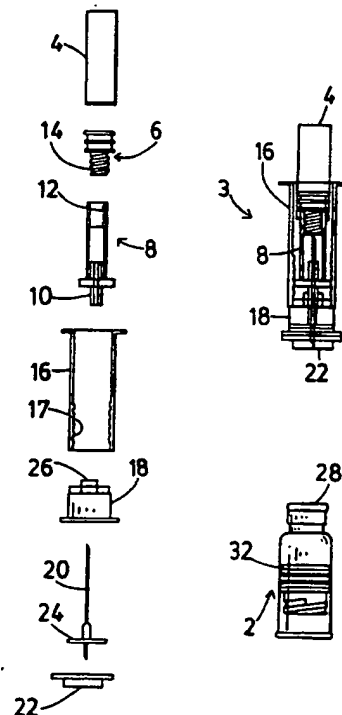

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	FR	France	MR	Mauritania
AU	Australia	GA	Gabon	MW	Malawi
BB	Barbados	GB	United Kingdom	NL	Netherlands
BE	Belgium	GN	Guinea	NO	Norway
BF	Burkina Faso	GR	Greece	NZ	New Zealand
BG	Bulgaria	HU	Hungary	PL	Poland
BJ	Benin	IE	Ireland	PT	Portugal
BR	Brazil	IT	Italy	RO	Romania
CA	Canada	JP	Japan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SK	Slovak Republic
CI	Côte d'Ivoire	LJ	Liechtenstein	SN	Senegal
CM	Cameroon	LK	Sri Lanka	SU	Soviet Union
CS	Czechoslovakia	LU	Luxembourg	TD	Chad
CZ	Czech Republic	MC	Monaco	TG	Togo
DE	Germany	MG	Madagascar	UA	Ukraine
DK	Denmark	ML	Mali	US	United States of America
ES	Spain	MN	Mongolia	VN	Viet Nam
FI	Finland				

- 1 -

SYRINGE

## TECHNICAL FIELD

This invention relates to prefilled syringe systems  
5 for the packaging of pharmaceutical preparations in dosage  
form, and more particularly to systems in which two  
components of a preparation, one of which is normally a  
diluent or solvent, must be stored separately and only  
admixed immediately prior to administration.

## 10 BACKGROUND ART

Our United States Patent No. 5,137,511 describes  
several syringe systems for the packaging of two component  
pharmaceutical preparations, of which the system shown in  
Figures 11 and 12 is presently the most preferred. This  
15 system stores a solvent or diluent component in a specially  
formed capsule 14 which is described in detail in that  
patent.

Shell vials are however a well known and widely  
available packaging for pharmaceutical diluents. A shell  
20 vial differs from a conventional pharmaceutical or serum  
vial in that it has no neck. Instead the top of the vial  
is of the same diameter as the remainder of the cylindrical  
side wall of the vial, and is closed by a piston quite  
similar to that utilized by the present applicant to close  
25 the bottom of its bottomless vial as described in U.S.  
Patent No. 5,137,511.

## DISCLOSURE OF INVENTION

I have now found that the construction shown in  
this patent can be advantageously modified to utilize known  
30 shell vials in place of the capsule 14.

According to the invention, a prefilled syringe  
system for two component pharmaceuticals is provided, as  
set forth in the appended claims 1-5.

- 2 -

## BRIEF DESCRIPTION OF DRAWINGS

Preferred embodiments of the invention are described with reference to the accompanying drawings, in which:

5            Figures 1A-1I are elevations illustrating successive stages in the assembly and preparation of use of a first embodiment of the invention, it being assumed for ease in illustration that most components other than those of rubber or metal are transparent; and

10           Figures 2A-2G are elevations illustrating successive stages in the assembly and preparation for use of a second embodiment of the invention.

## BEST MODES FOR CARRYING OUT THE INVENTION

Figure 1A shows an exploded view of the components  
15 of a separately assembled and sterilized unit 3 (see Figure 1B) for use in conjunction with a filled and capped vial 2 generally similar to that shown in Figure 12 of U.S. Patent No. 5,137,511. The unit 3 comprises a shell vial having a cylindrical body 4 closed at one end, and a piston 6  
20 closing its other end to enclose a quantity of pharmaceutical diluent. A moulded plastic tubular adaptor component 8 has a tubular connector 10 at one end similar to the connector element 70 of U.S. Patent No. 5,137,511, and an internal thread 12 within its other end forms a  
25 coupling engaged with an external thread on an extension 14 forming a coupling configuration on the piston 6. A tubular plunger 16 has an internal thread 17 which can provide a coupling to an integral extension or other coupling configuration on a piston 32 of the vial 2. This  
30 plunger and a cap 18 are similar to corresponding parts shown in the U.S. patent. The unit further includes a cannula needle 20, and a protective cap 22 which closes the open end of the cap 18 to maintain sterility and provide protection of the needle during storage. The cap 22 is

- 3 -

removed immediately before use (see Figure 1C). The needle 20 is of the double ended type, and is located beneath the cap 18 by a flange 24. A connector 26 on the cap engages the connector 10 on the adaptor component 8 in the same way as the connector 27 engages the connector 70 in Figure 12 of U.S. Patent No. 5,137,511, so that one end of the needle 20 passes through the adaptor towards the piston extension 14, as seen in Figure 1B.

After the cap 22 has been removed (Figure 1C), as well as a flip-off protective cover 28 on the cap 30 of the vial 2, which protects a rubber closure of the vial held in place by the cap 30 (Figure 1F), the unit 3 is pressed onto the vial 2 (Figure 1F) so that the cap 18 is pressed over the cap 30 of the vial 2 so that the lower end of the needle 20 pierces a rubber closure of the vial 2. At the same time, the flange 24 is pressed upwardly within the cap 18 and causes the upper end of the needle 20 to penetrate a septum within the piston 6.

The shell vial 4 is then pressed downwardly (Figure 7F) expelling its contents through the needle 20 into the vial 2. If necessary, the piston 32 within the vial 2 is positioned higher in the vial than normal so that it can be displaced downwardly to make room for the contents of vial 4 (see Figure 1G).

At this point, the assembly 3, with the exception of the cap 18 and the needle 20, is pulled away from the vial 2 by gripping the plunger 16 leaving the cap and needle in place on the vial (Figure 1G). The thread 17 of plunger 16 is then screwed onto the piston 32 of the vial 2 (Figure 1H) to form a syringe 34 (Figure 1I).

In the embodiment just described, the shell vial is dimensioned so as to fit within the tubular plunger. An

- 4 -

alternative embodiment is shown in Figures 2A-G in which the shell vial 4 is dimensioned so that the tubular plunger 16 has an external diameter less than its internal diameter. The same reference numerals are used to denote those components of this embodiment which are similar to those of the previous embodiment, and only the differences will be described. In this instance, the plunger 16 fulfils the functions of the adaptor 8, the screw threads on extensions of the pistons 6 and 32 being similar except that the thread 14 on piston 6 may be longer. The plunger 16 is a press fit on the connector 26 on the cap 18, which in this case is formed with a skirt 36 which fits over the top portion of the vial 2 and also provides a finger grip 38. The entire unit 3 (see Figure 2C) is assembled into a tubular sleeve 40 (Figure 2B) which together with the cap 22 maintains sterility of the unit during storage, and also facilitates preparation of the syringe. The vial 4 is a press fit within the upper end of the sleeve 40. After removal of the cap 22, the unit 3 is applied to the vial (Figure 2D) as in the previous embodiment, and the sleeve 40 is pulled downwardly (Figure 2E). As before, this forces the cap 18 onto the cap 30 of the vial, causing the needle 20 to pierce both the closure of the vial 2 and the piston 6 of the shell vial 4, and further downward movement of the sleeve 40 forces the contents of the shell vial into the vial 2. At this point the sleeve 40 is rotated to unscrew the piston 6 of the shell vial 4 from the plunger 16 (Figure 2F) which is then transferred to the piston 32 to complete the syringe.

It should be understood that the sleeve 40 could be omitted, although it is a convenience for packaging and manipulating the syringe, in which case the vial 4 would be manipulated directly rather than through the sleeve 40.

- 5 -

Variations in the above embodiments are possible. For some applications of the syringe, it may be desired to replace the needle 20 by some other cannula arrangement when the syringe is used, in which case a single ended  
5 needle may be located in the assembly 3 so that it will be forced upwardly as the cap 18 is forced onto the vial 2 (the cap in this case will have an internal cannula to pierce the closure of the vial), but will be retained within the shell vial when the latter is removed during  
10 preparation of the syringe. If a double ended needle 30 is used, in combination with a cannula, venting of the vial 2 to permit escape of air displaced by the contents of the shell vial 4 becomes possible, in a manner similar to that shown in Figure 16 of U.S. Patent No. 5,137,511.

- 6 -

CLAIMS:

1. A prefilled syringe system for two component pharmaceuticals, characterized by the combination of first and second subassemblies, of which the first subassembly comprises a bottomless pharmaceutical vial (2) having a filling neck, a penetrable closure retained on said neck by a first annular cap (30), and an open bottom end hermetically closed by a first piston (32) with a downwardly facing coupling configuration within the vial, and the second subassembly (3) comprises a shell vial (4) having an open end closed by a second piston (6), a tubular plunger (16) concentric and in telescoping relationship with the shell vial, the plunger having a coupling (17) at one end for subsequent coupling to the coupling configuration (14) of said first piston (32), a second cap (18) releasably connected to said plunger which can be force fitted to said first cap (30), and cannula means (20) projectable by force fitting of said first cap (30) to said second cap (18) to penetrate both said penetrable closure and said second piston (6) to place said bottomless vial (2) and said shell vial (4) in fluid communication through said cannula means (20) whereby fluid from the shell vial is transferred to the bottomless vial upon telescoping said shell vial relative to said plunger (16).

2. A syringe system according to claim 1, characterized in that the shell vial (4) is of a diameter to telescope into said plunger (16), and adaptor means (8) are provided in said second subassembly extending between said second cap (18) and a coupling configuration (14) on said second on said second piston (6) to maintain the position of the latter during telescoping of the shell vial relative to the plunger.

**SUBSTITUTE SHEET**

- 7 -


3. A syringe system according to claim 1, characterized in that the shell vial (4) is of a diameter to telescope around said plunger (16), and said means (17) on the plunger for coupling to the coupling configuration of the first piston (32) are initially coupled to coupling means (14) on the second piston (6).

4. A syringe according to claim 3, characterized in that the components of the second subassembly (3) are assembly within a tubular housing (40), and the shell vial (4) is a press fit within the tubular housing.

5. A syringe system according to any one of claims 1-4, characterized in that the cannula means (20) is a double ended needle, with a flange (24) to control its longitudinal position received within the second cap (18).

**SUBSTITUTE SHEET**

1/4

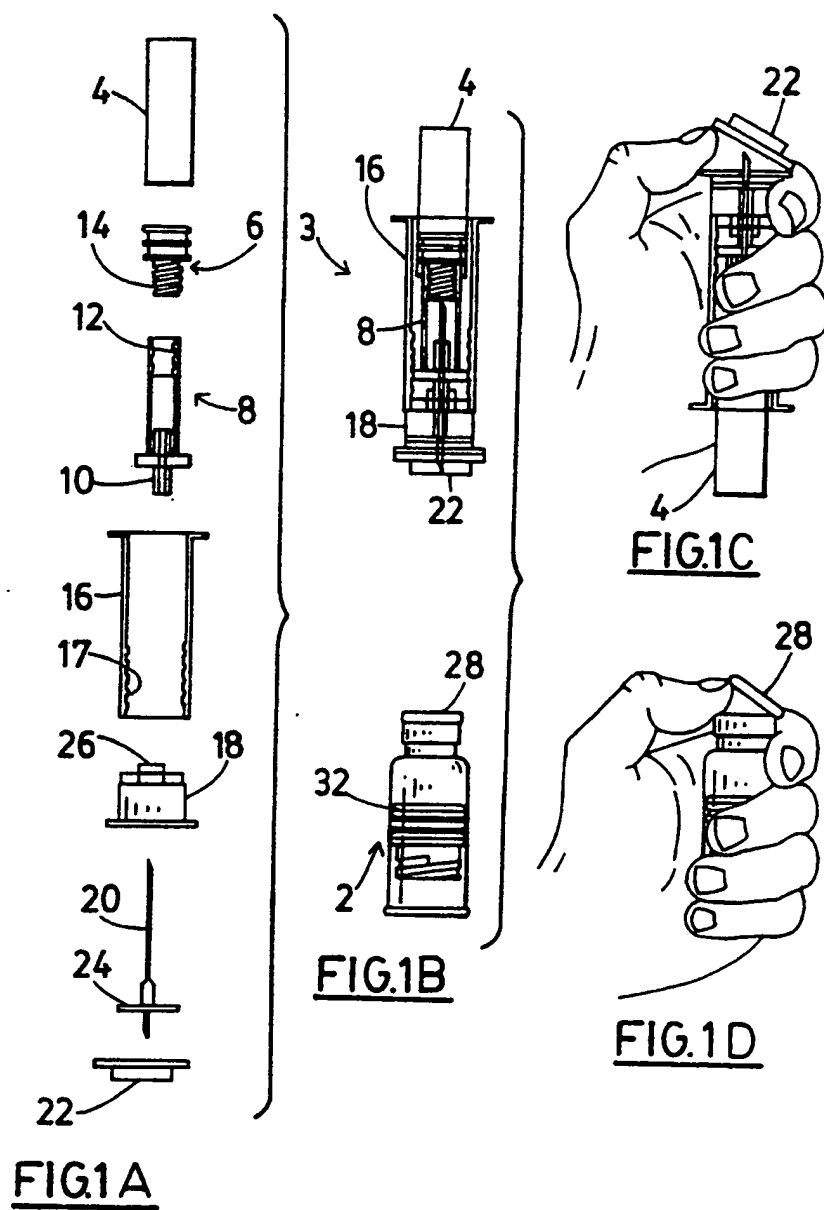

2/4

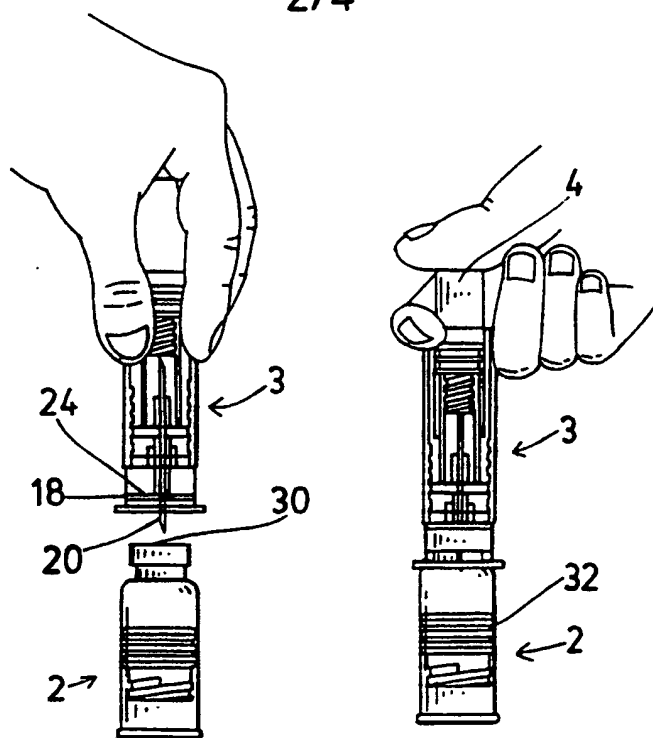


FIG. 1E

FIG. 1F

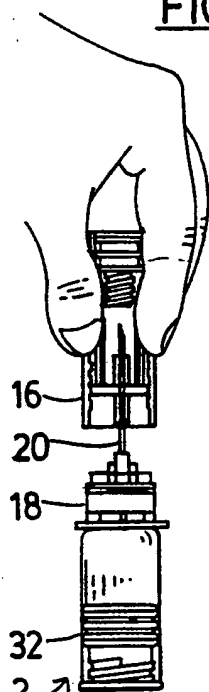


FIG. 1G

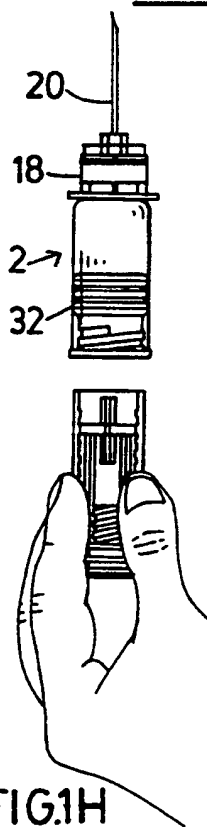


FIG. 1H

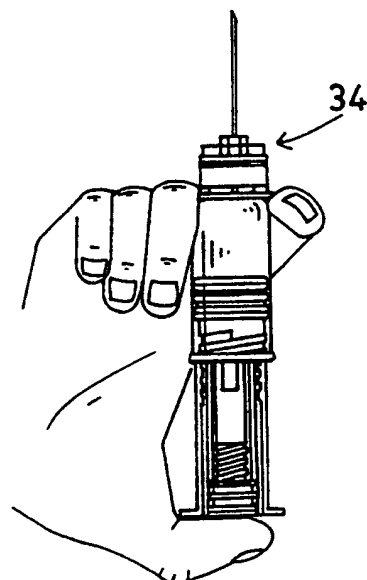


FIG. 1I

3/4

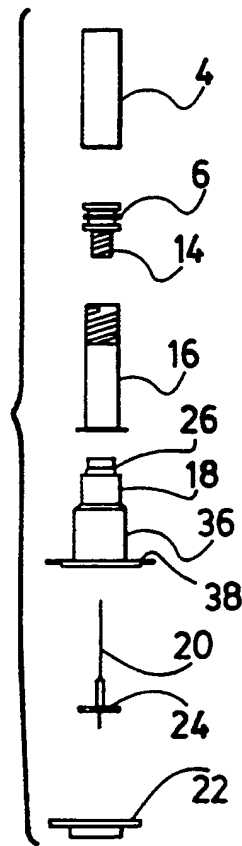


FIG. 2A

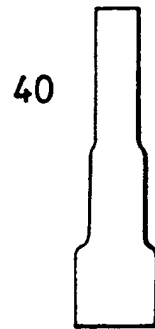


FIG. 2B

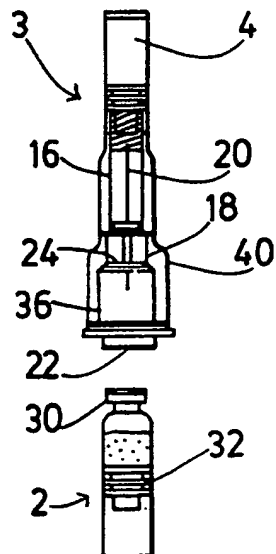


FIG. 2C




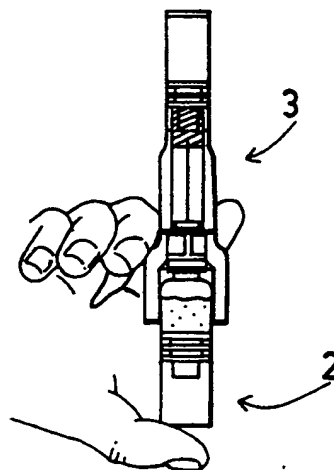


FIG. 2D

4/4

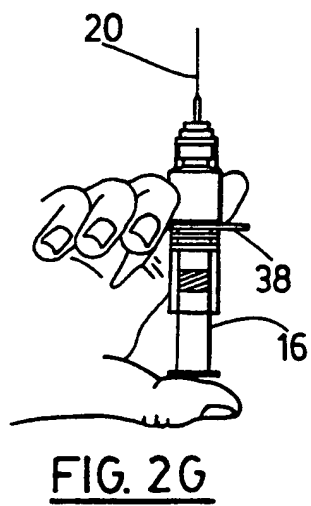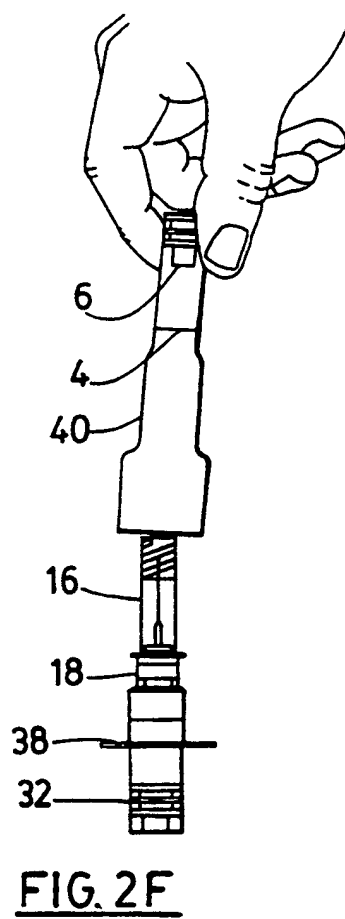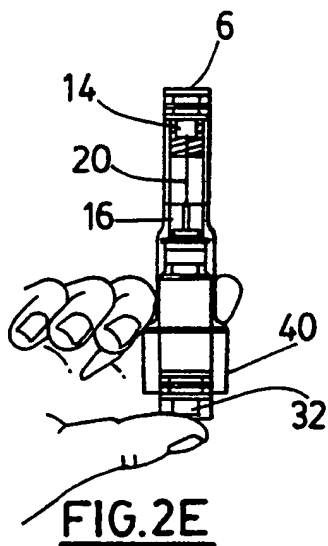

## INTERNATIONAL SEARCH REPORT

International Application No

PCT/CA 92/00495

<b>I. CLASSIFICATION OF SUBJECT MATTER</b> (If several classification symbols apply, indicate all) <sup>6</sup>		
According to International Patent Classification (IPC) or to both National Classification and IPC		
Int.Cl. 5 A61M5/28		
<b>II. FIELDS SEARCHED</b>		
Minimum Documentation Searched <sup>7</sup>		
Classification System	Classification Symbols	
Int.Cl. 5	A61M ; A61J	
Documentation Searched other than Minimum Documentation to the Extent that such Documents are Included in the Fields Searched <sup>8</sup>		
<b>III. DOCUMENTS CONSIDERED TO BE RELEVANT<sup>9</sup></b>		
Category <sup>10</sup>	Citation of Document, <sup>11</sup> with indication, where appropriate, of the relevant passages <sup>12</sup>	Relevant to Claim No. <sup>13</sup>
A	EP,A,0 298 585 (DUOJECT MEDICAL SYSTEMS INC) 11 January 1989 see the whole document	1,2,5
A,P	& US,A,5 137 511 (REYNOLDS) cited in the application	
A	DE,A,1 766 151 (FARBENFABRIKEN BAYER AG) 3 June 1971 see claims; figure 2	1
A	US,A,4 424 057 (HOUSE) 3 January 1984 see claims; figures	1
A	US,A,4 014 330 (GENESE) 29 March 1977 see claims; figures	1
<p><sup>10</sup> Special categories of cited documents : <sup>10</sup></p> <p>"A" document defining the general state of the art which is not considered to be of particular relevance</p> <p>"E" earlier document but published on or after the international filing date</p> <p>"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</p> <p>"O" document referring to an oral disclosure, use, exhibition or other means</p> <p>"P" document published prior to the international filing date but later than the priority date claimed</p> <p>"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</p> <p>"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step</p> <p>"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.</p> <p>"&amp;" document member of the same patent family</p>		
<b>IV. CERTIFICATION</b>		
Date of the Actual Completion of the International Search		Date of Mailing of this International Search Report
11 MARCH 1993		16. 03. 93
International Searching Authority		Signature of Authorized Officer
EUROPEAN PATENT OFFICE		SEDY R.

**ANNEX TO THE INTERNATIONAL SEARCH REPORT  
ON INTERNATIONAL PATENT APPLICATION NO.**

CA 9200495  
SA 66152

This annex lists the patent family members relating to the patent documents cited in the above-mentioned international search report.  
The members are as contained in the European Patent Office EDP file on  
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information. 11/03/93

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
EP-A-0298585	11-01-89	US-A- 4886495	12-12-89
		AU-B- 623594	21-05-92
		CA-A- 1295525	11-02-92
		GB-A- 2210268	07-06-89
		JP-A- 1131671	24-05-89
		US-A- 5137511	11-08-92
-----			
DE-A-1766151	03-06-71	None	
-----			
US-A-4424057	03-01-84	None	
-----			
US-A-4014330	29-03-77	AU-B- 500379	17-05-79
		AU-A- 1810176	06-04-78
		BE-A- 847695	27-04-77
		CA-A- 1058035	10-07-79
		CH-A- 612350	31-07-79
		DE-A- 2648795	03-11-77
		FR-A, B 2329296	27-05-77
		GB-A- 1562637	12-03-80
		NL-A- 7611905	02-05-77
		SE-B- 428264	20-06-83
		SE-A- 7611963	30-06-77
-----			